


Vein clamp monitoring with Aïmago ResearchLDI



A	Perfusion before vein clamp, average value: 182
B	Artifact due to clamp insertion on vein by surgeon
C	Perfusion after clamp on vein, average value: 100
D	Artifact due to flap movement during clamp search and removal by surgeon
E	Perfusion 10s after clamp, average value: 111
F	Measurement interruption
G	Artifact due to flap movement during flap touching and moving by surgeon
H	Perfusion 2min after vein clamp, average value: 121

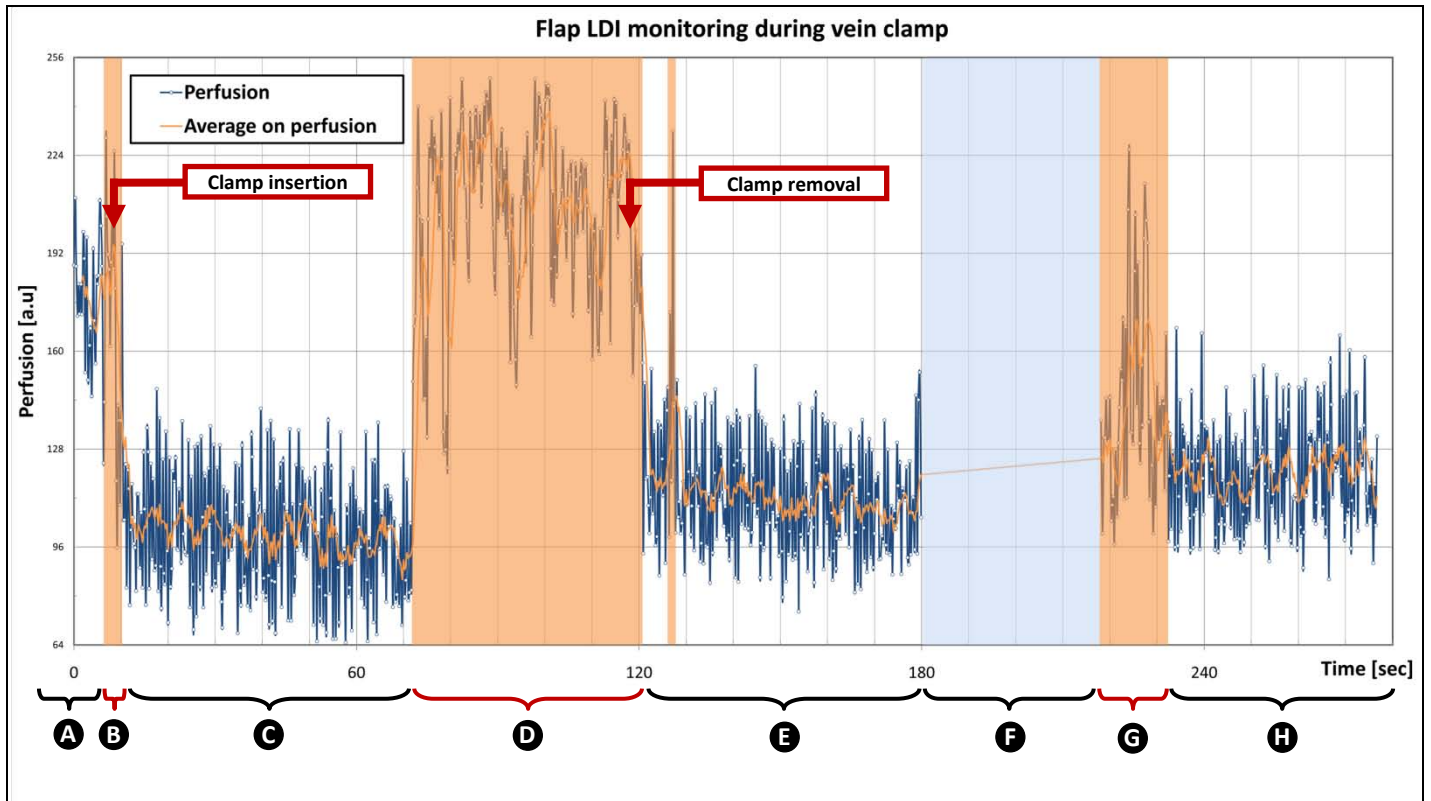